

FIG. 1A

WO 2004/096082 PCT/US2004/012758

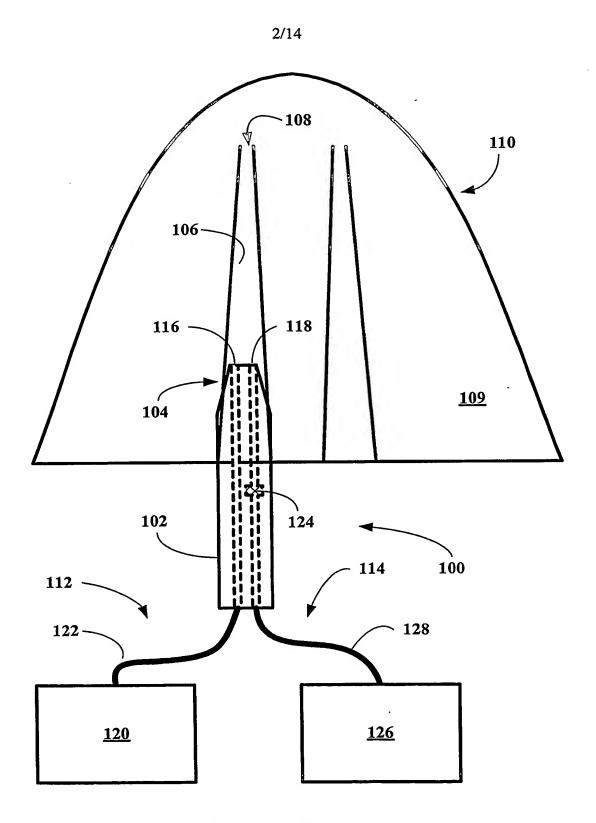


FIG. 1B

WO 2004/096082 PCT/US2004/012758

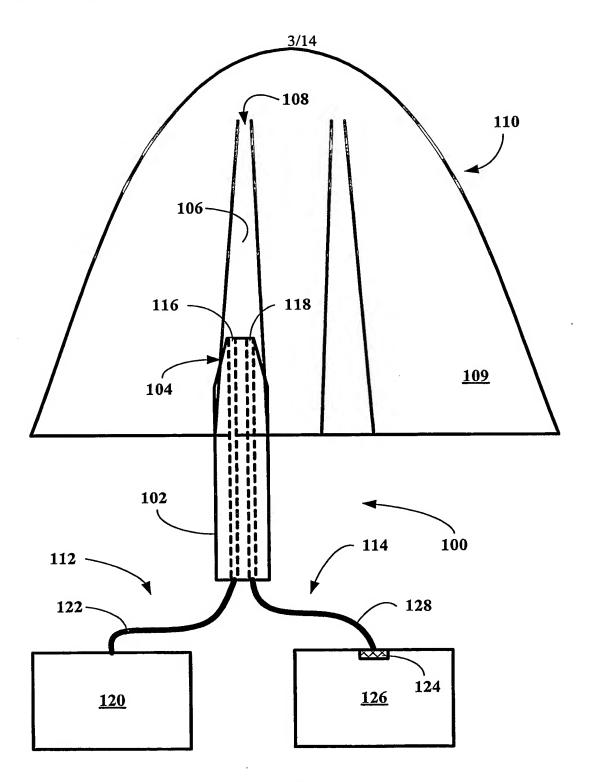
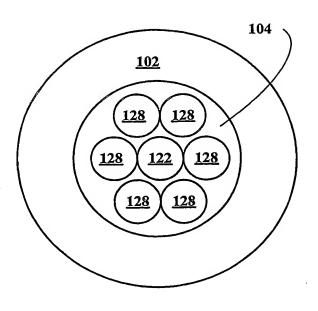


FIG. 1C

4/14






FIG. 1D

102

104

128 128 122 122

128 128 122 122

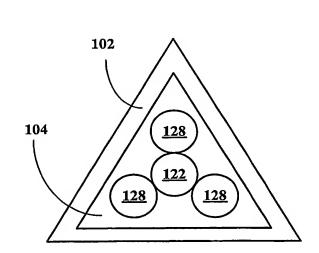


FIG. 1E

FIG. 1G

5/14

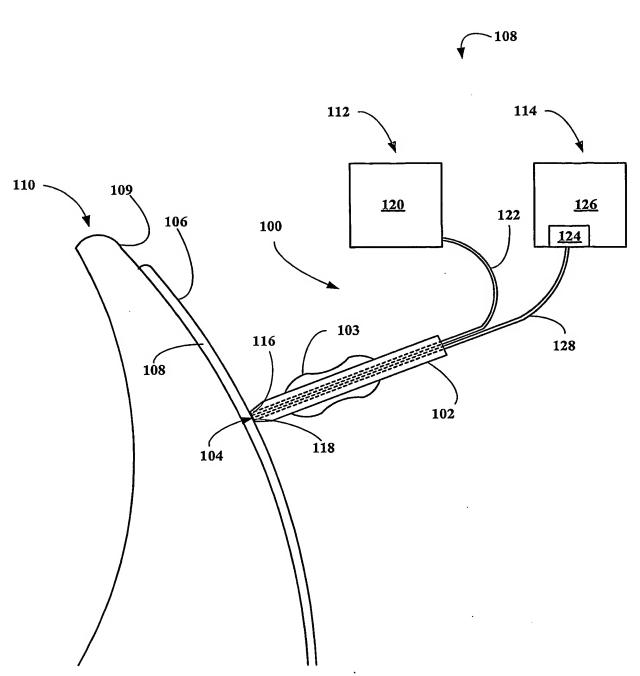


FIG. 1H



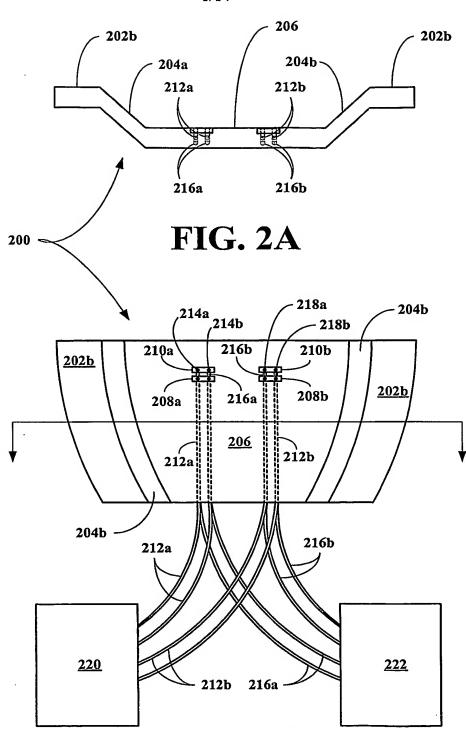


FIG. 2B

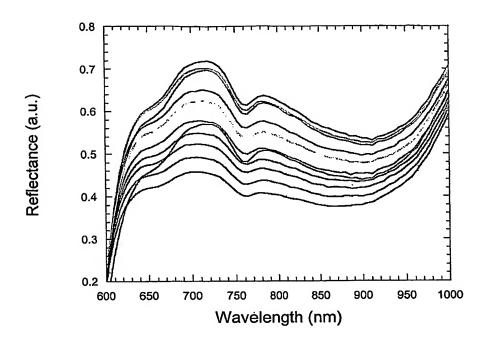


FIG. 3

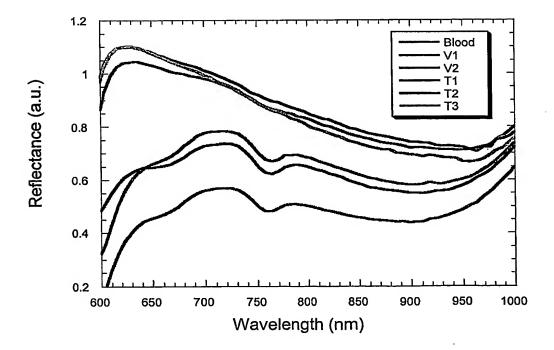


FIG. 4

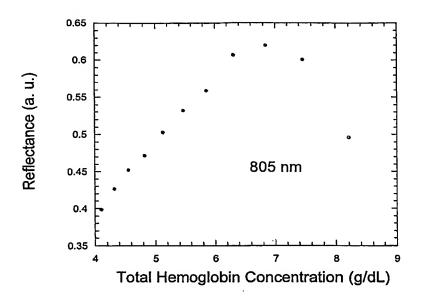


FIG. 5

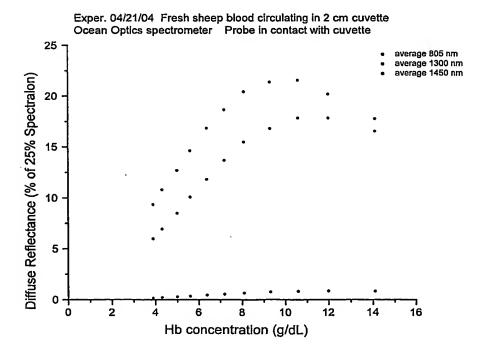


FIG. 6A

Exper. 04/21/04 Fresh sheep blood circulating in 2 cm cuvette Ocean Optics spectrometer Probe in contact with cuvette

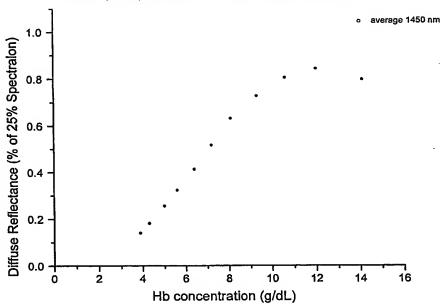


FIG. 6B

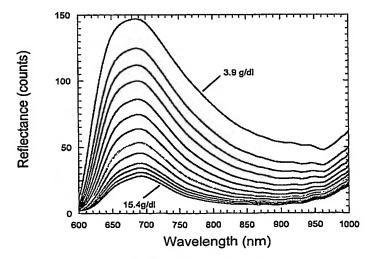


FIG. 7A

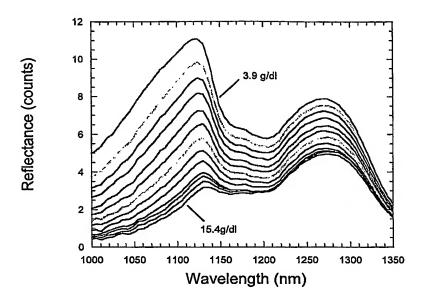


FIG. 7B

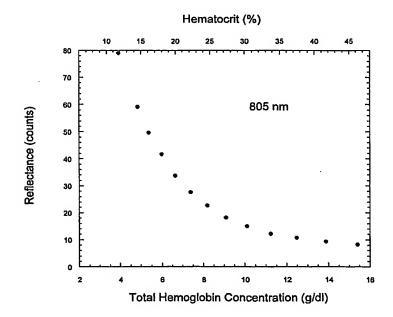


FIG. 8A

WO 2004/096082 PCT/US2004/012758

11/14

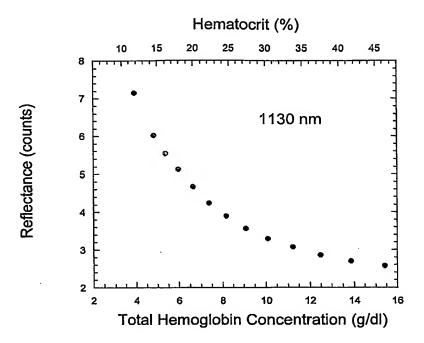


FIG. 8B

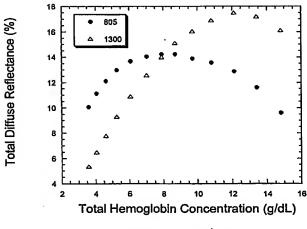


FIG. 9A




FIG. 9B

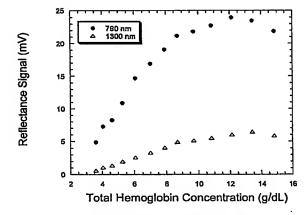


FIG. 10A

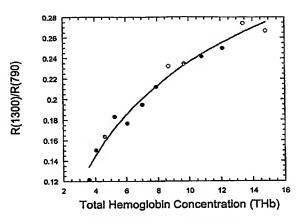


FIG. 10B

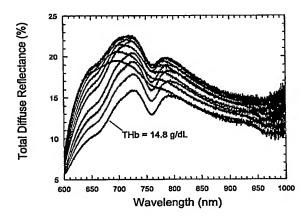


FIG. 11A

PCT/US2004/012758

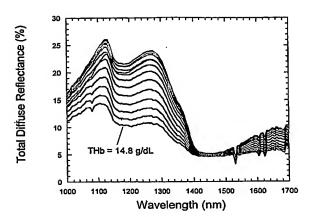


FIG. 11B

.

WO 2004/096082